

BEST AVAILABLE COPY

1/8

Initial Assay Using Dendritic Capture Reagents Single Channel

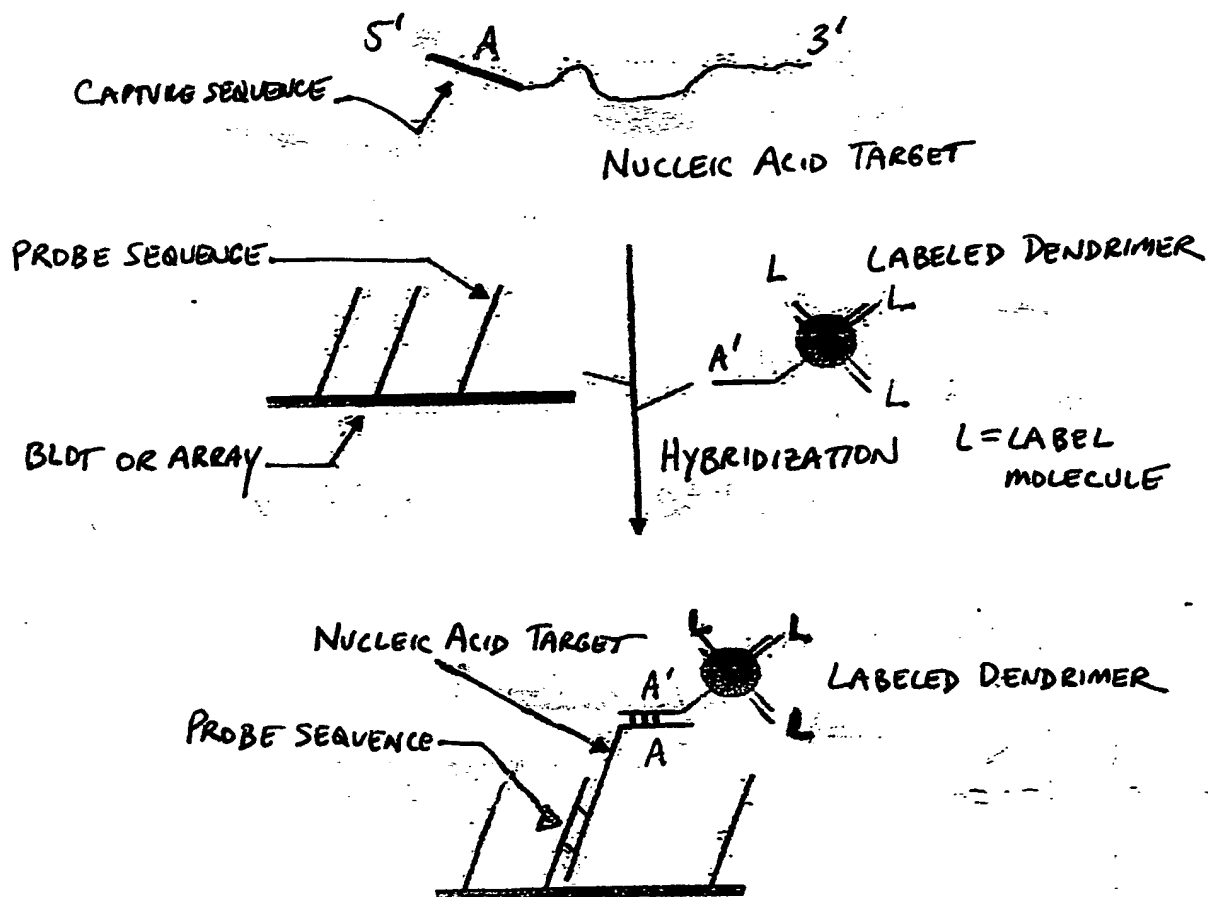


FIGURE 1

2/8

Stripping of the Blot/Array Single Channel

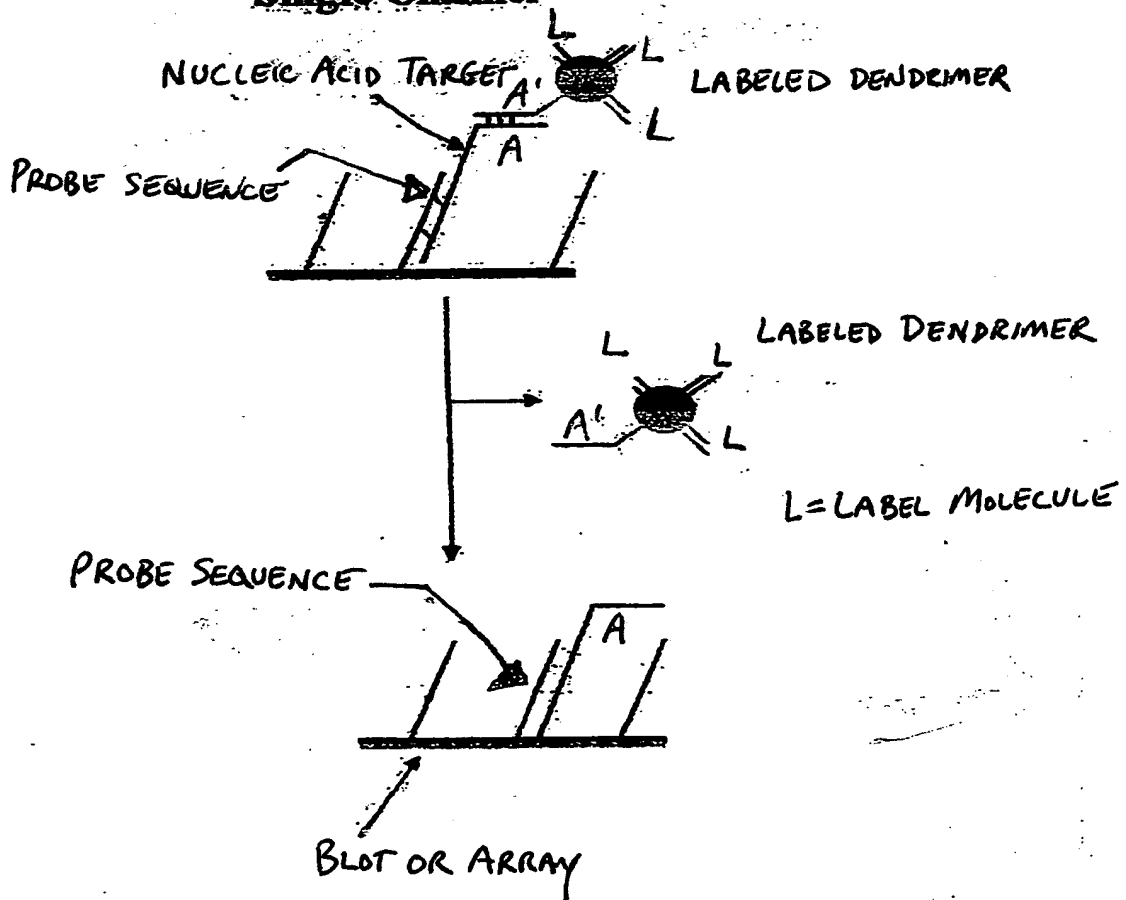


FIGURE 2

3/8

Repeat Assay Using Dendritic Capture Reagents Single Channel

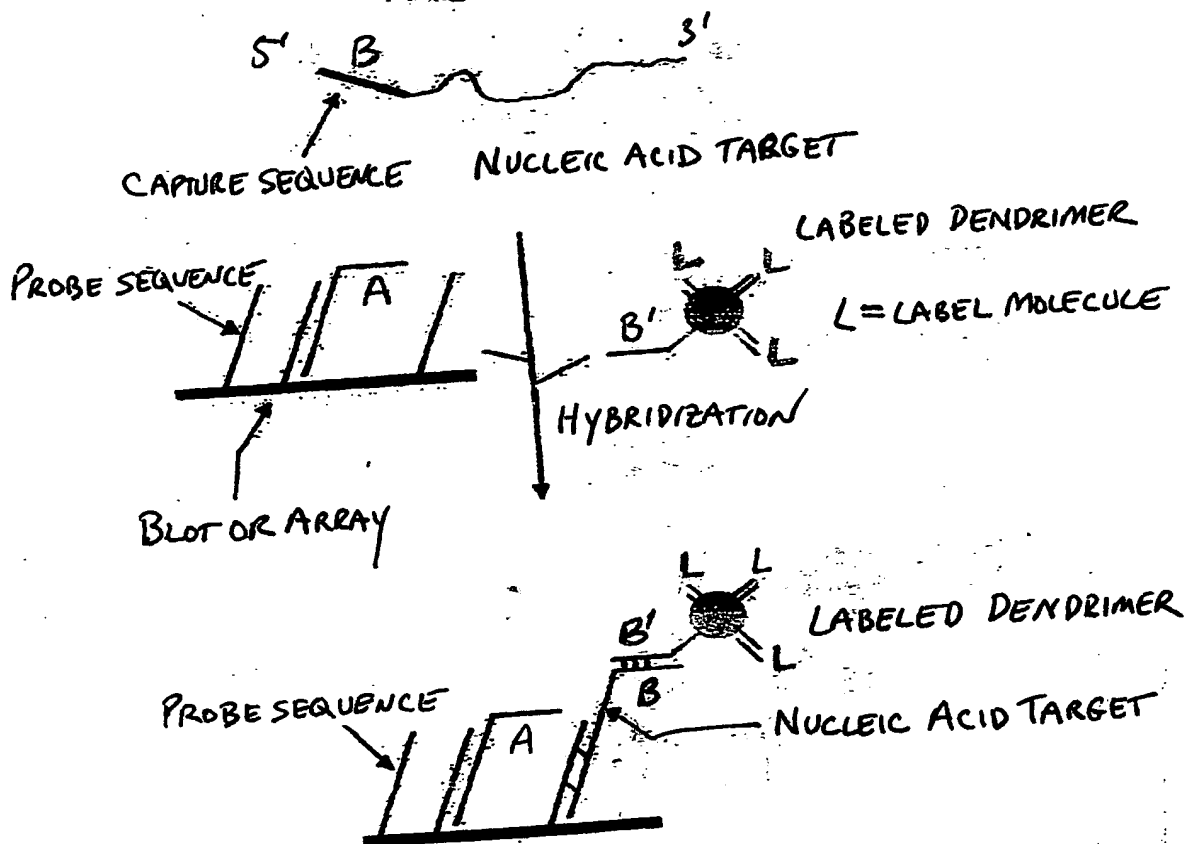


FIGURE 3

4/8

Initial Assay Using Dendritic Capture Reagents Double Channel

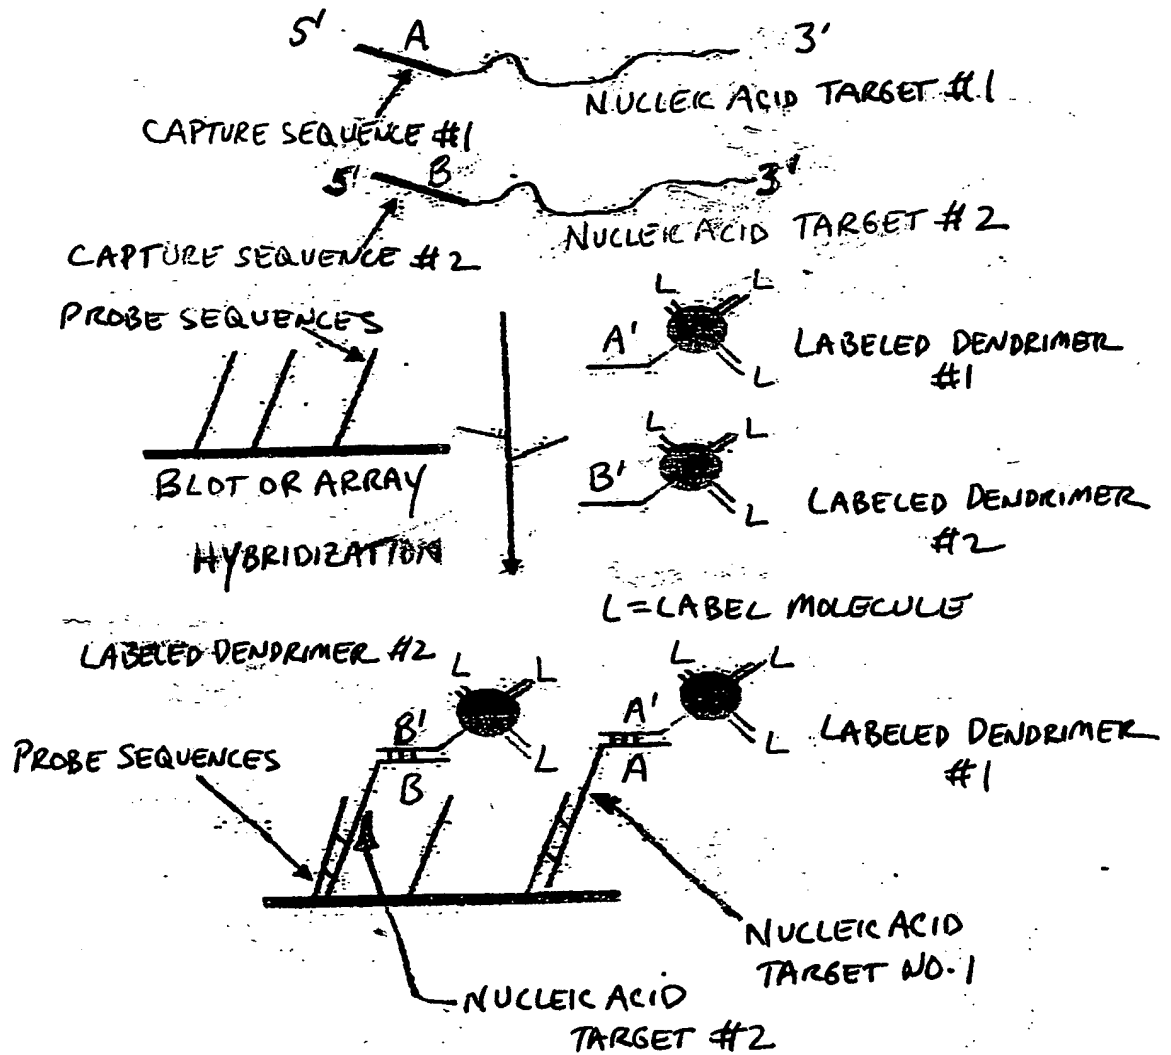


FIGURE 4

5/8

Stripping of Blot/Array Double Channel

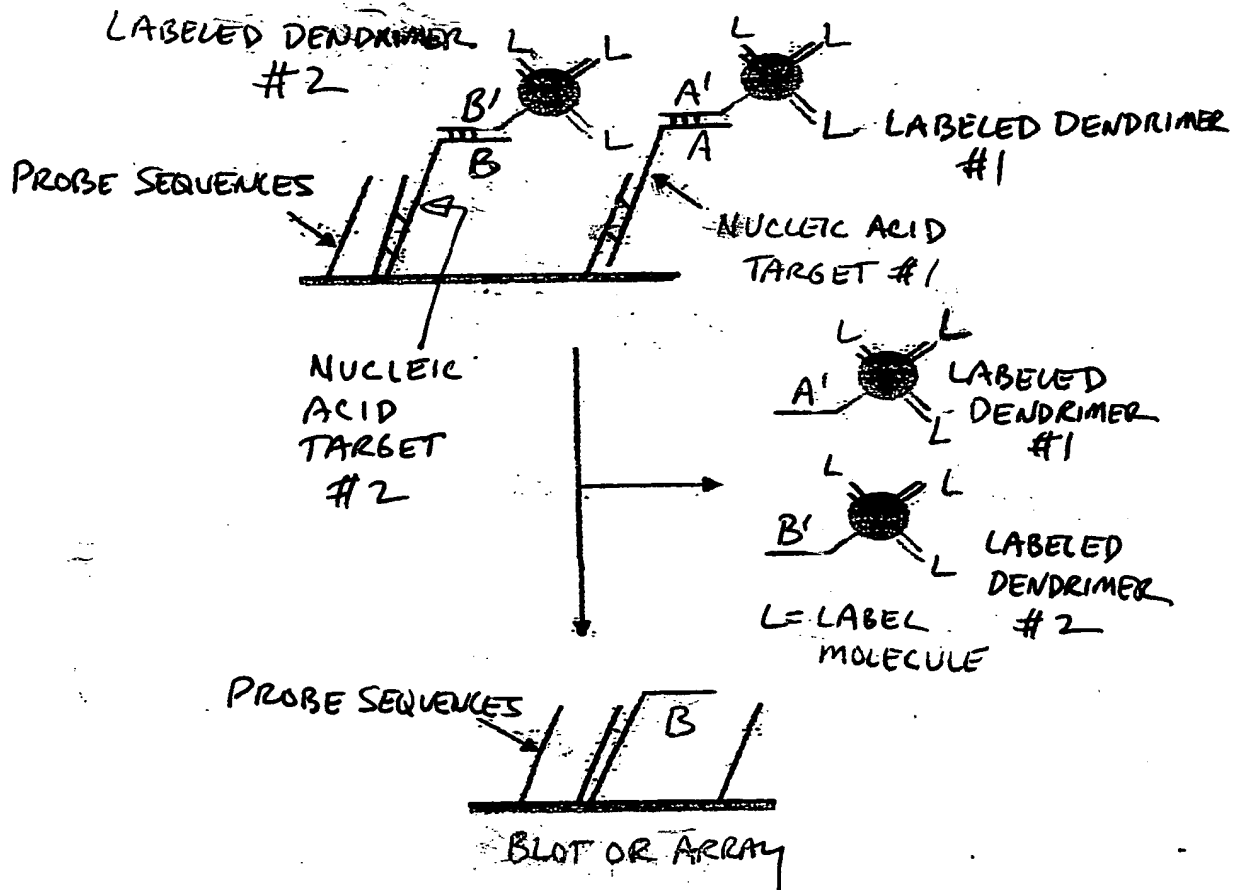


FIGURE 5

6/8

Repeat Assay Using Dendritic Capture Reagents Double Channel

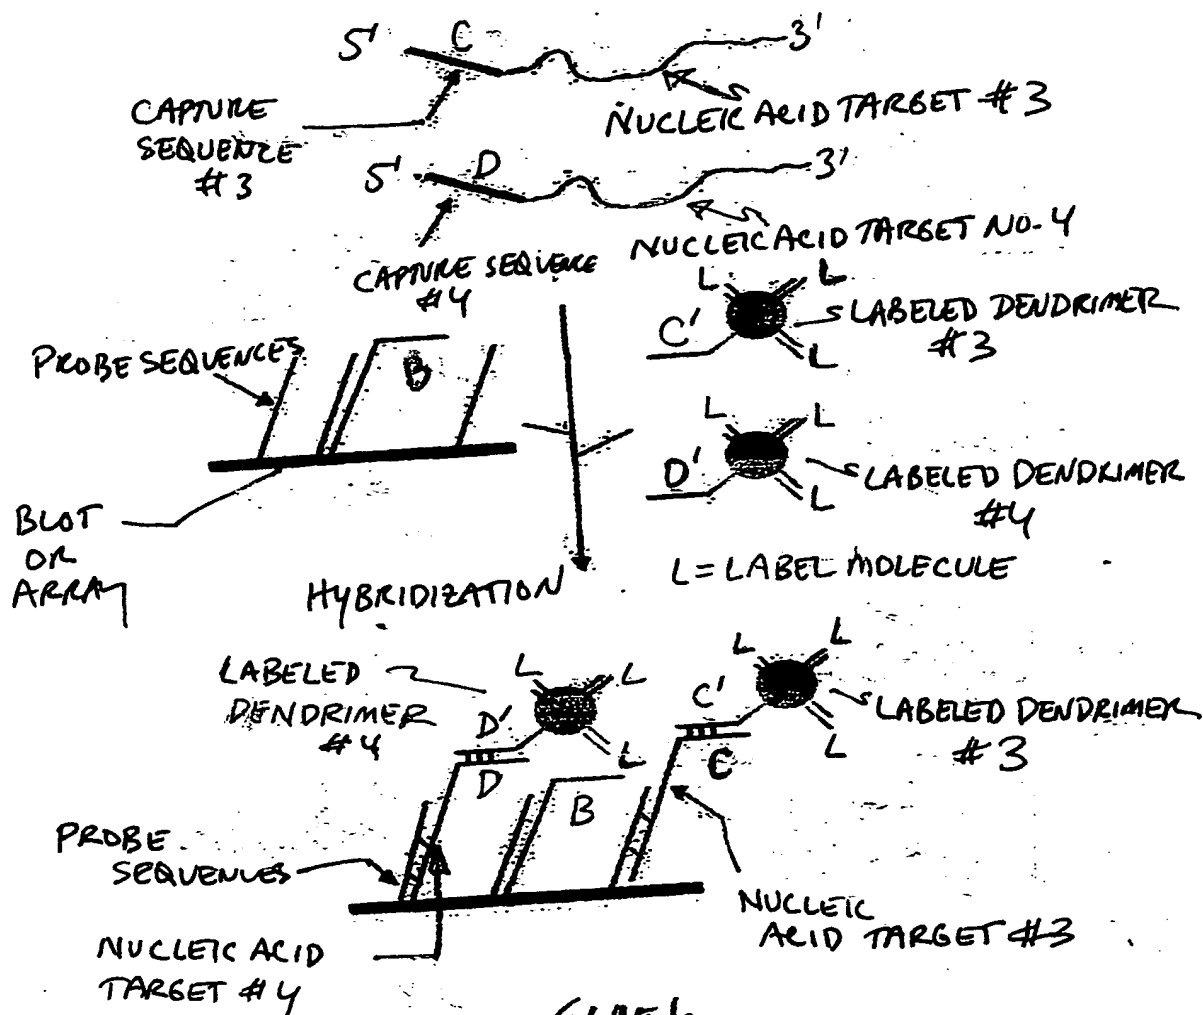


FIGURE 6

8/8

MICROARRAY DETECTION WITH DENDRITIC REAGENTS

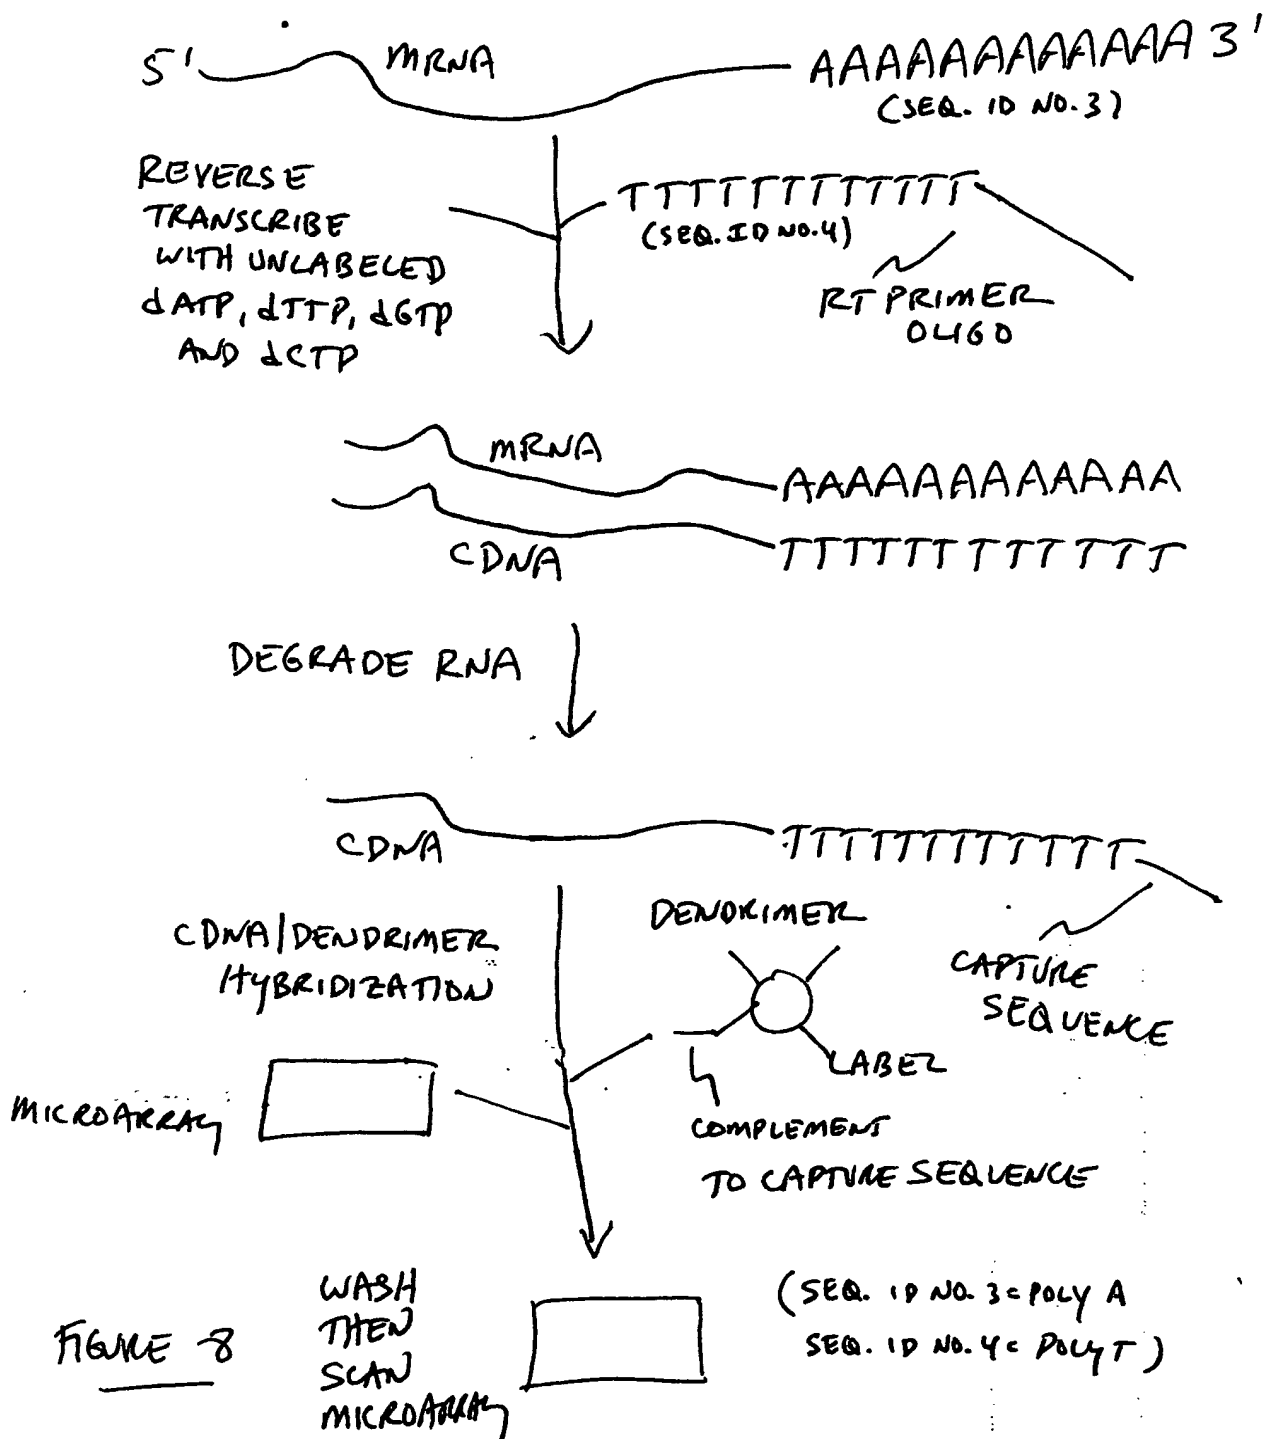


FIGURE 8